

# ESi / Premium Drill Sequence


## ∅ 3.5 Hex or NP High Stability Drill Sequence

For questions call manufacturer

Drill speed: 850-950 RPM

Torque: 40-50 Ncm

Important: Do not go above 45 NCM, if you did, please reverse to an 1/8 - 1/4 of a turn.

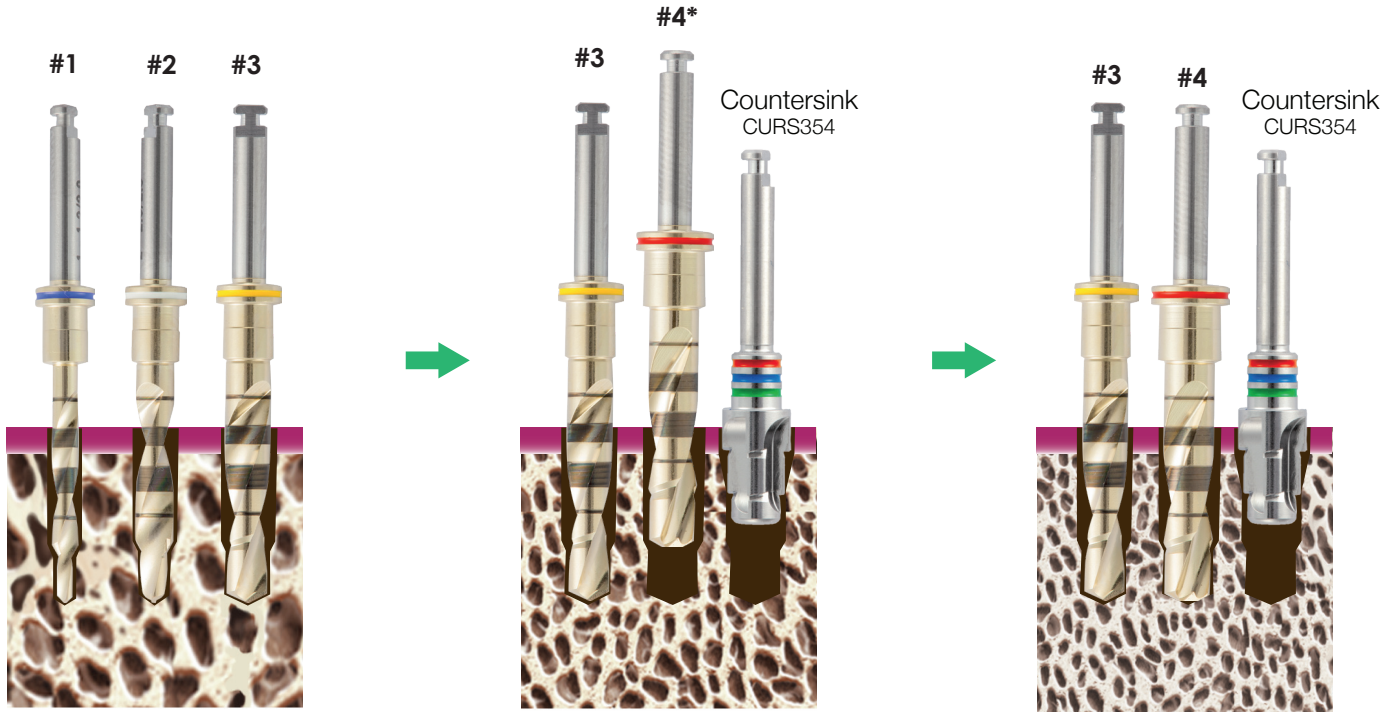


Type 4 & 3 Bone

Type 2 Bone

Type 1 Bone

Note: For ∅3.5 implants the crestal diameter is 3.7mm. Therefore, for bone types 1 & 2, countersink **must be used**.

## ∅ 4.3 Hex or RP

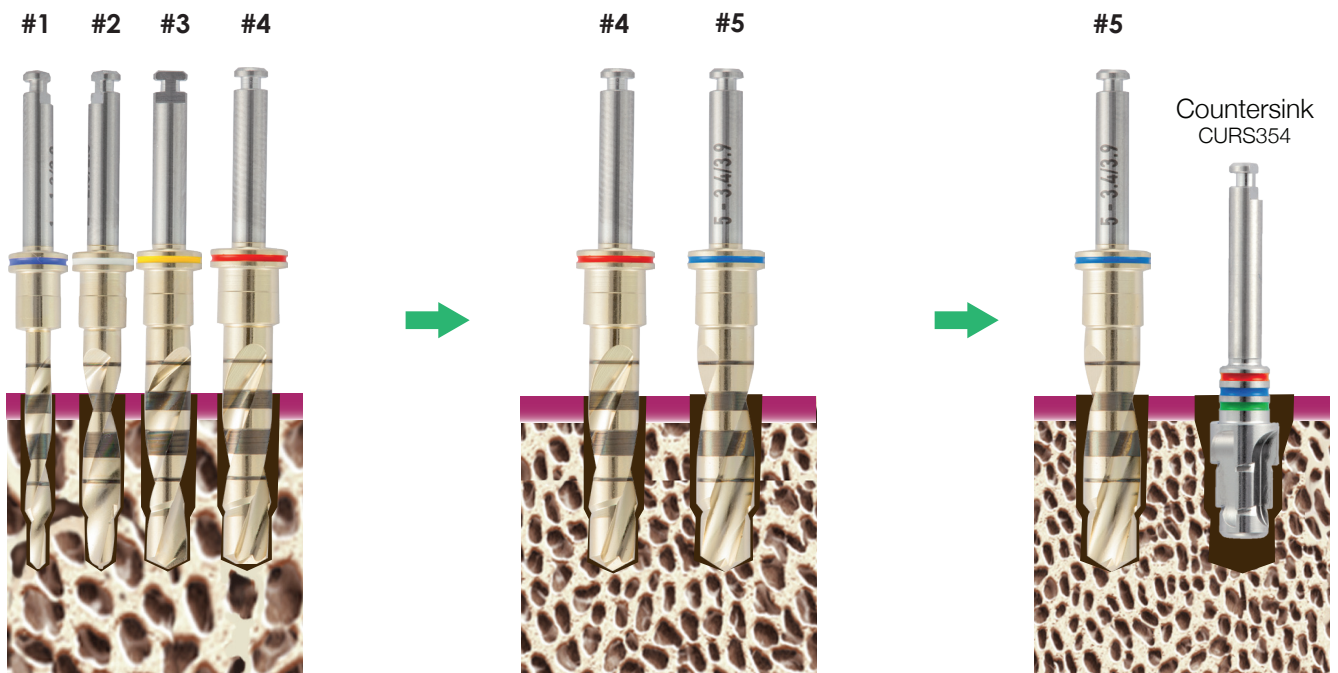

Type 3, 4 Bone

Type 2 Bone

Type 1 Bone

# ESi / Premium Drill Sequence

## Ø 3.5 Hex or NP High Stability Drill Sequence

For questions call manufacturer

Drill speed: 850-950 RPM

Torque: 40-50 Ncm

Important: Do not go above 45 NCM, if you did, please reverse to an 1/8 - 1/4 of a turn.



Type 4 & 3 Bone



Type 2 Bone



Type 1 Bone

Note: For Ø3.5 implants the crestal diameter is 3.7mm. Therefore, for bone types 1 & 2, countersink **must be used**.


## Ø 4.3 Hex or RP



Type 3, 4 Bone



Type 2 Bone

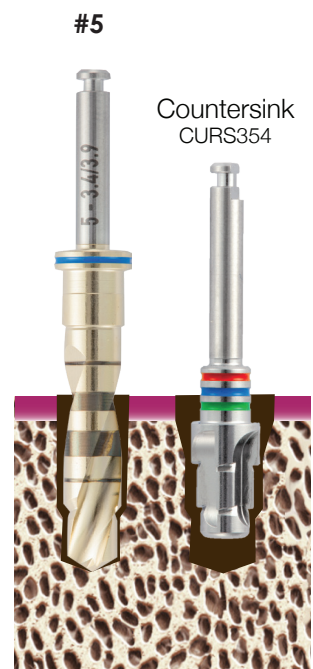


Type 1 Bone

# ESi / Premium Drill Sequence

Drill speed: 850-950 RPM

Torque: 35-40 Ncm

.....  
ø 5.0 Hex or RP

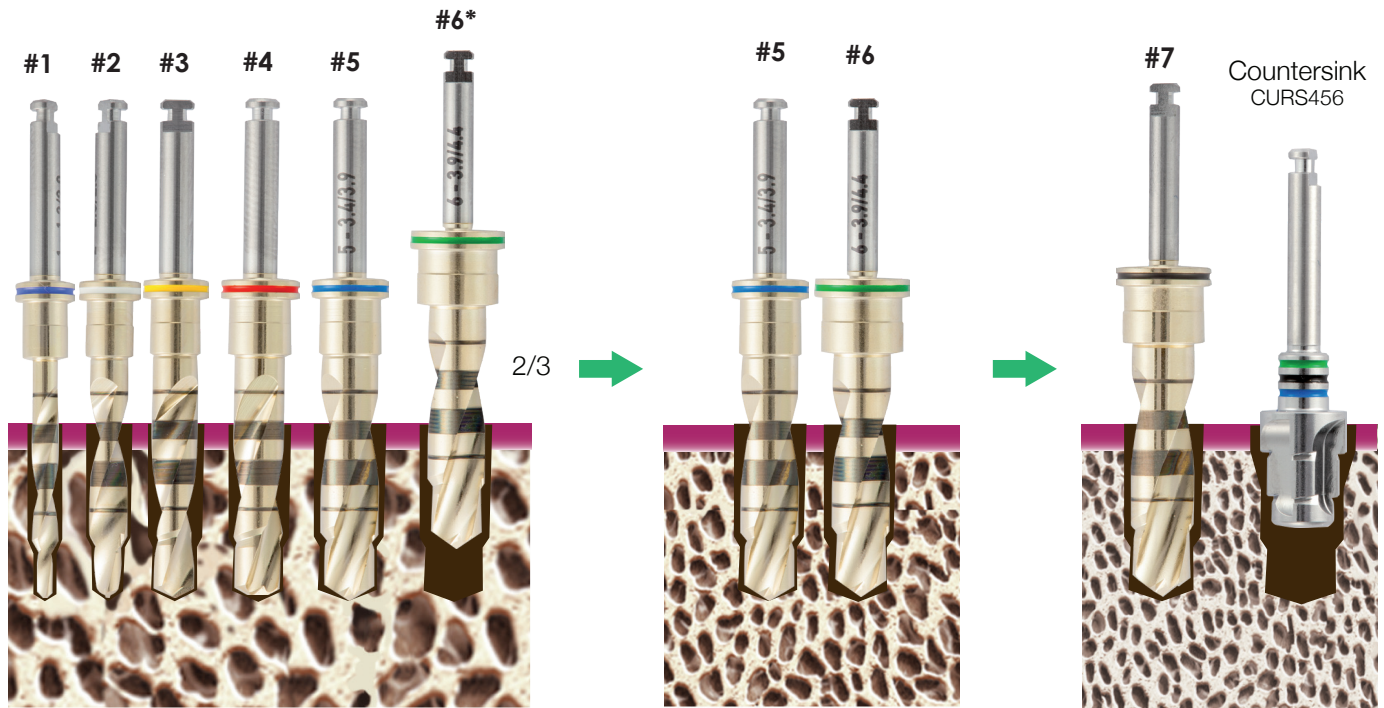


Type 4 & 3 Bone

Type 2 Bone

Type 1 Bone

ø 6.0 Hex or RP

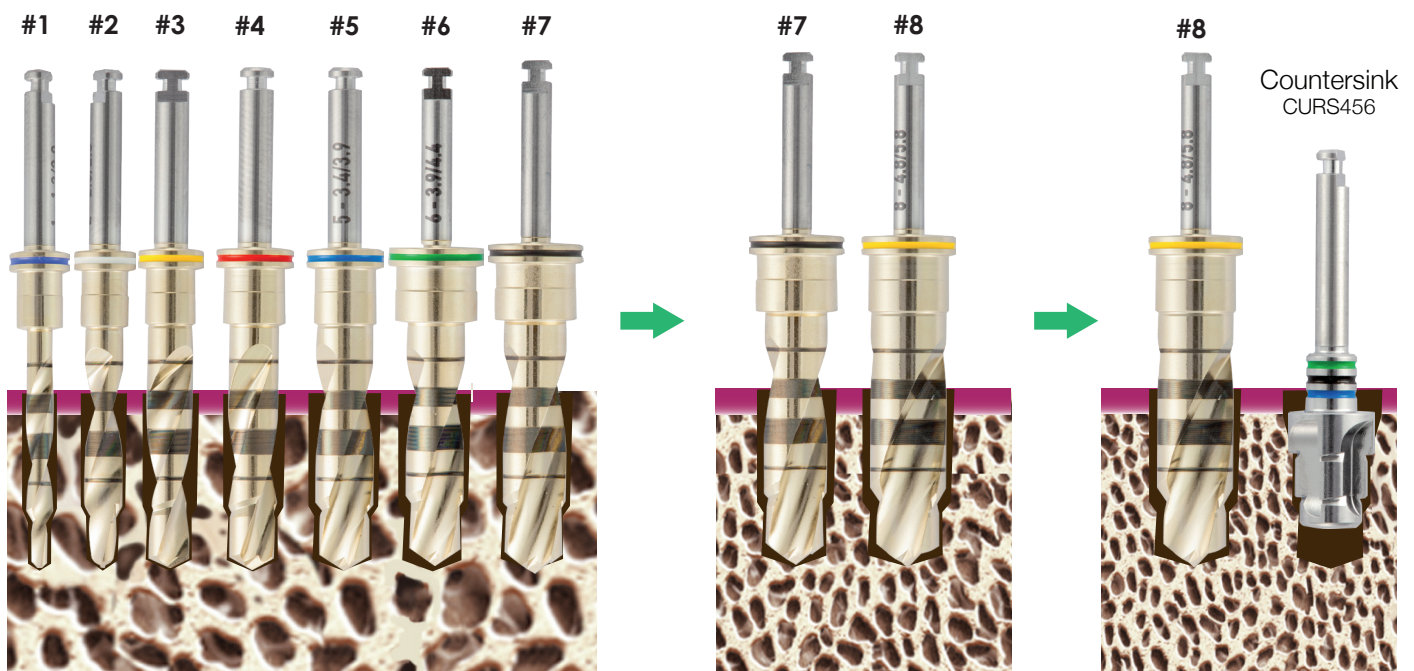

Type 4 & 3 Bone

Type 2 Bone

Type 1 Bone


Note: Make sure you are at least 1.5mm away from Inferior Alveolar Nerve or Sinus Floor.

# ESi / Premium Drill Sequence

Drill speed: 850-950 RPM

Torque: 35-40 Ncm

.....  
Ø 5.0 Hex or RP

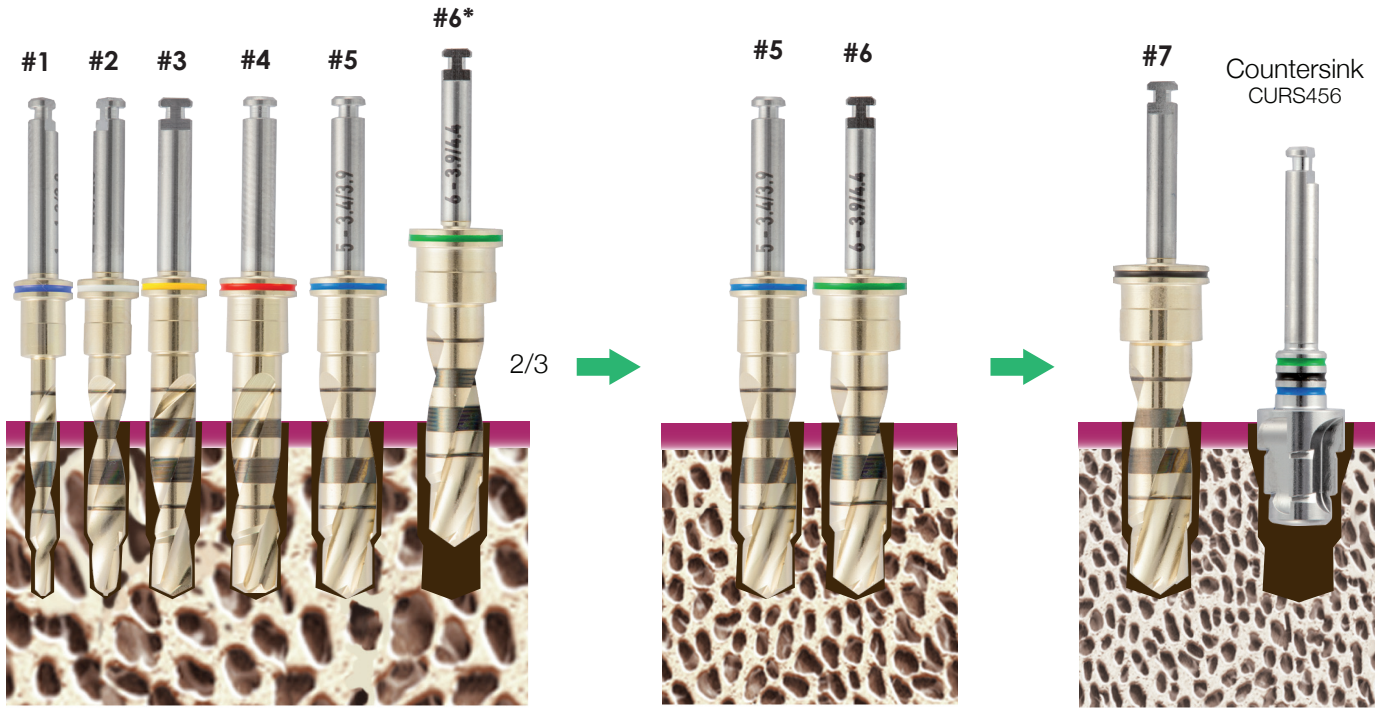


Type 4 & 3 Bone

Type 2 Bone

Type 1 Bone

Ø 6.0 Hex or RP

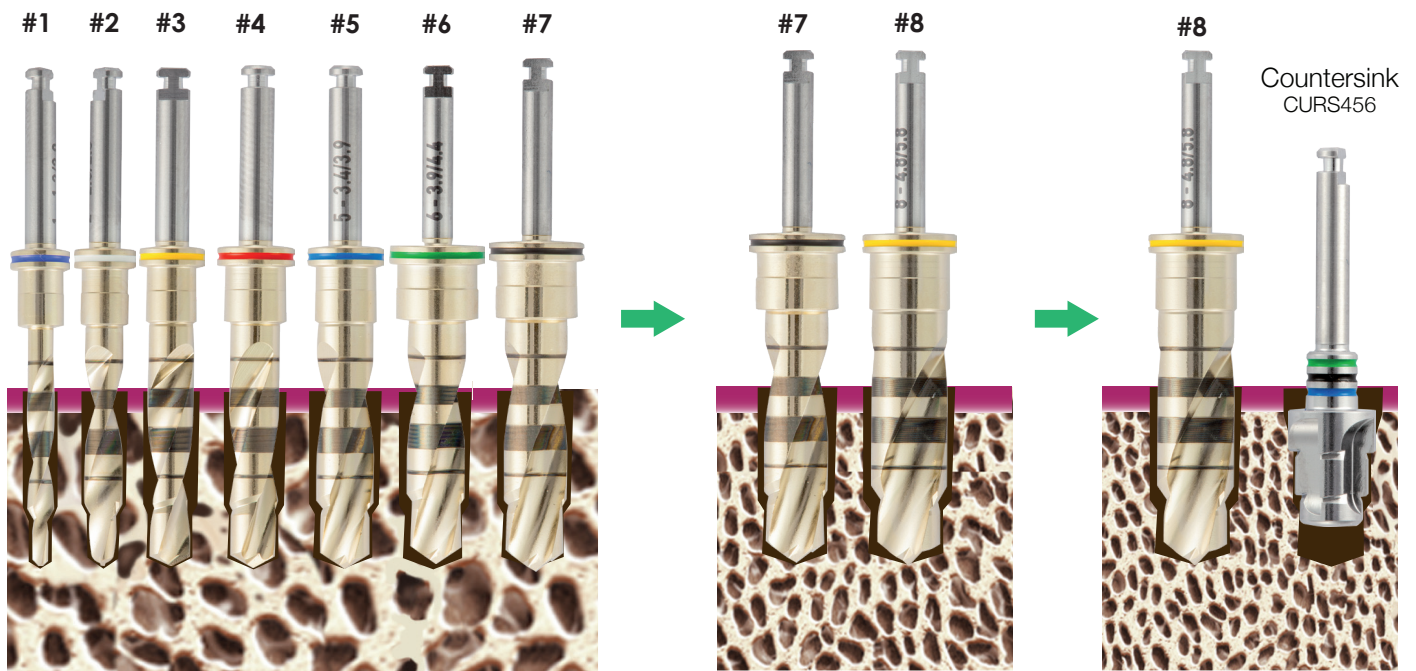

Type 4 & 3 Bone

Type 2 Bone

Type 1 Bone

Note: Make sure you are at least 1.5mm away from Inferior Alveolar Nerve or Sinus Floor.